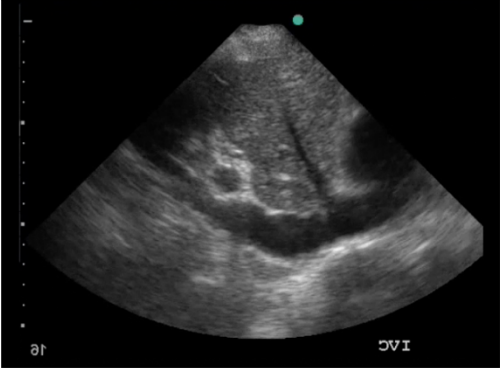
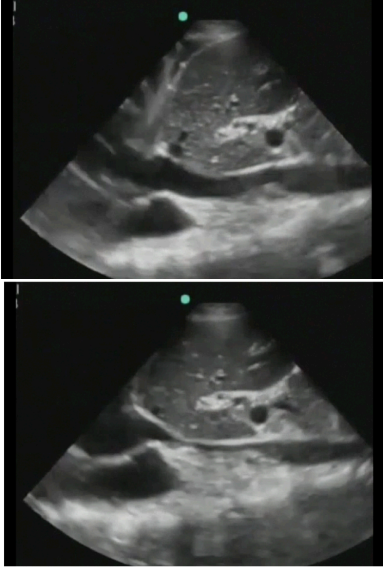
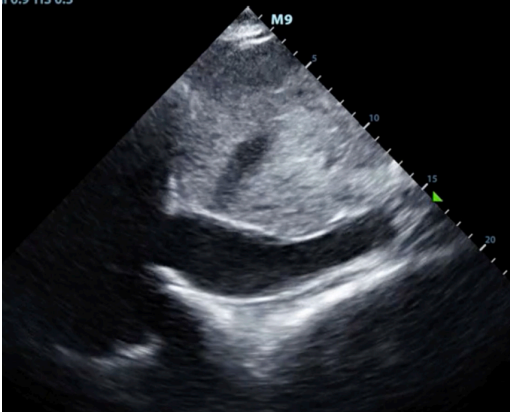
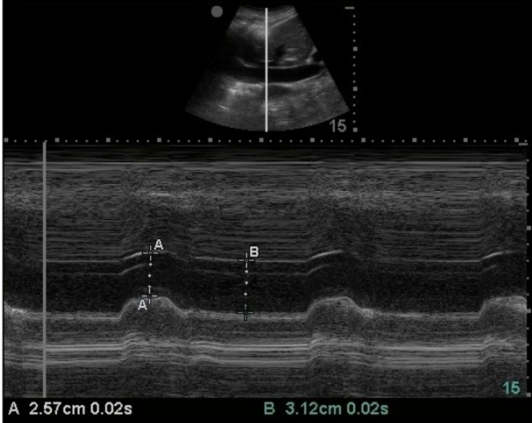


## Volume Assessment Reference Guide

IVC Diameter	Inspiratory Collapse (M-Mode or visualized)?	Estimated CVP	Fluid responsiveness?
<b>&lt;1.5 cm</b>	<b>Complete</b>	<b>&lt;5</b>	<b>Yes</b>
			
<b>&gt;2.5 cm</b>	<b>None</b>	<b>&gt;20</b>	<b>No</b>
			

Excerpt From: Matthew Dawson & Mike Mallin. "Introduction to Bedside Ultrasound: Volume 1." Emergency Ultrasound Solutions, 2013. iBooks.  
<https://books.apple.com/us/book/introduction-to-bedside-ultrasound-volume-1/id554196012>